

Display Report

Analysis Info



Analysis Name D:\Data\test0922\binghaoneizhi_4_01_1794.d
Method 1794.m
Sample Name binghaoneizhi
Comment

Acquisition Date 9/22/2014 9:39:47 AM

Operator bruker
Instrument amazon SL

Acquisition Parameter

Ion Source Type	ESI	Ion Polarity	Positive	Alternating Ion Polarity	on
Mass Range Mode	UltraScan	Scan Begin	100 m/z	Scan End	1000 m/z
Capillary Exit	140.0 V	Averages	n/a	Trap Drive	63.9
Accumulation Time	3621 μ s		3 Spectra	Auto MS/MS	off

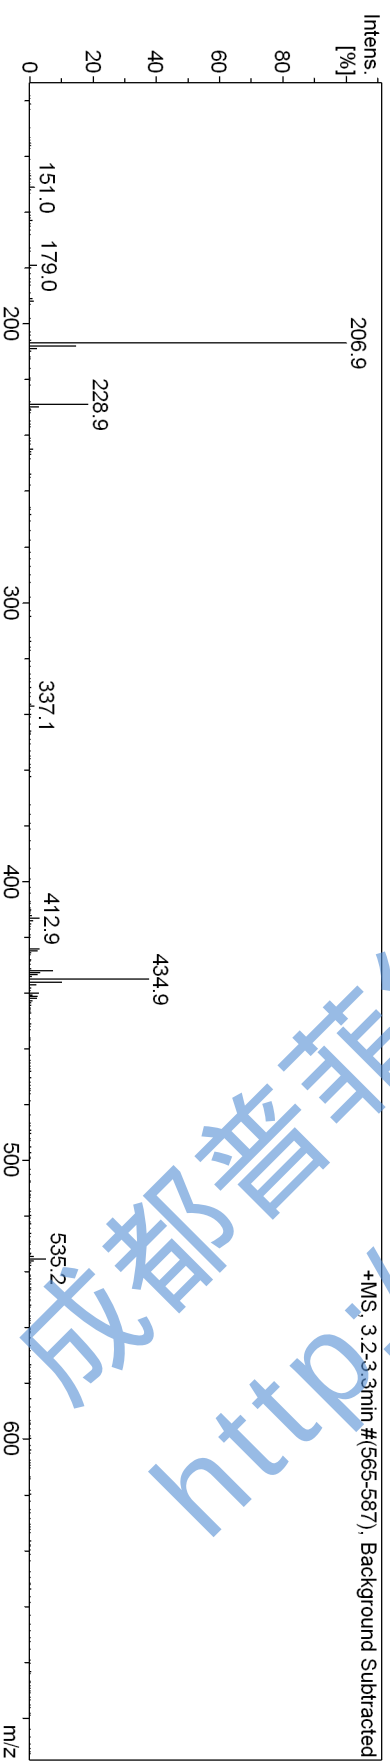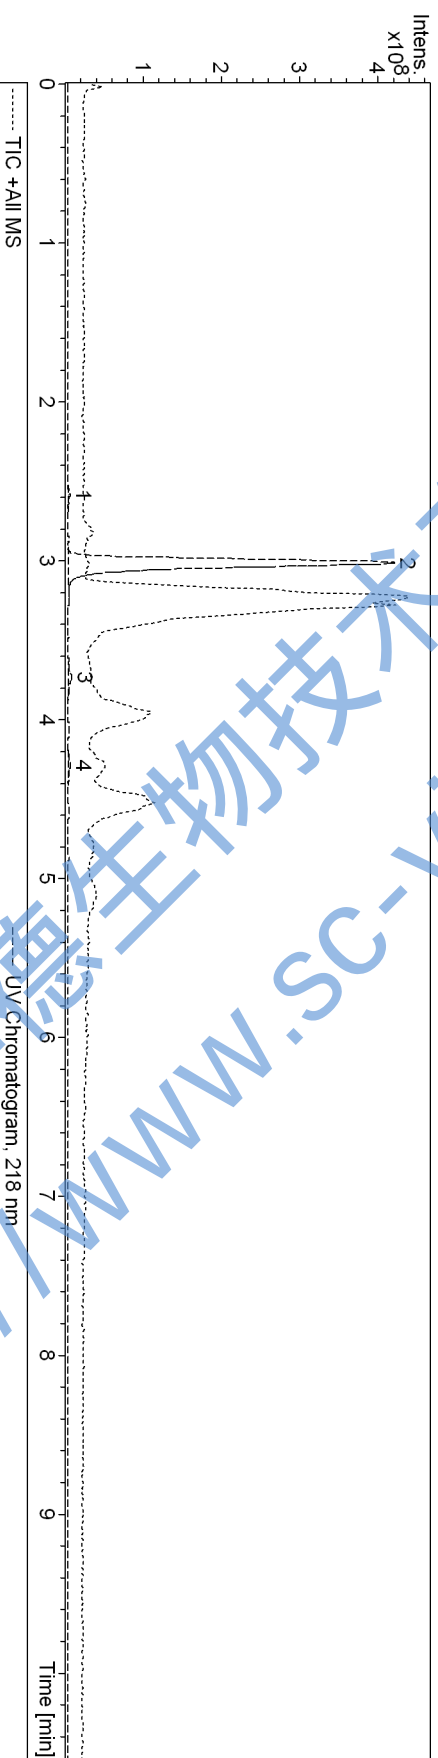

Display Report

Analysis Info


Analysis Name D:\Data\test\0922\binghaoneizhi_4_01_1794.d
 Method 1794.m
 Sample Name binghaoneizhi
 Comment

Acquisition Date 9/22/2014 9:39:47 AM

Operator bruker
 Instrument amazon SL

Acquisition Parameter

Ion Source Type	ESI	Ion Polarity	Positive	Alternating Ion Polarity	on
Mass Range Mode	UltraScan	Scan Begin	100 m/z	Scan End	1000 m/z
Capillary Exit	140.0 V	Averages	n/a	Trap Drive	63.9
Accumulation Time	3621 μ s		3 Spectra	Auto MS/MS	off

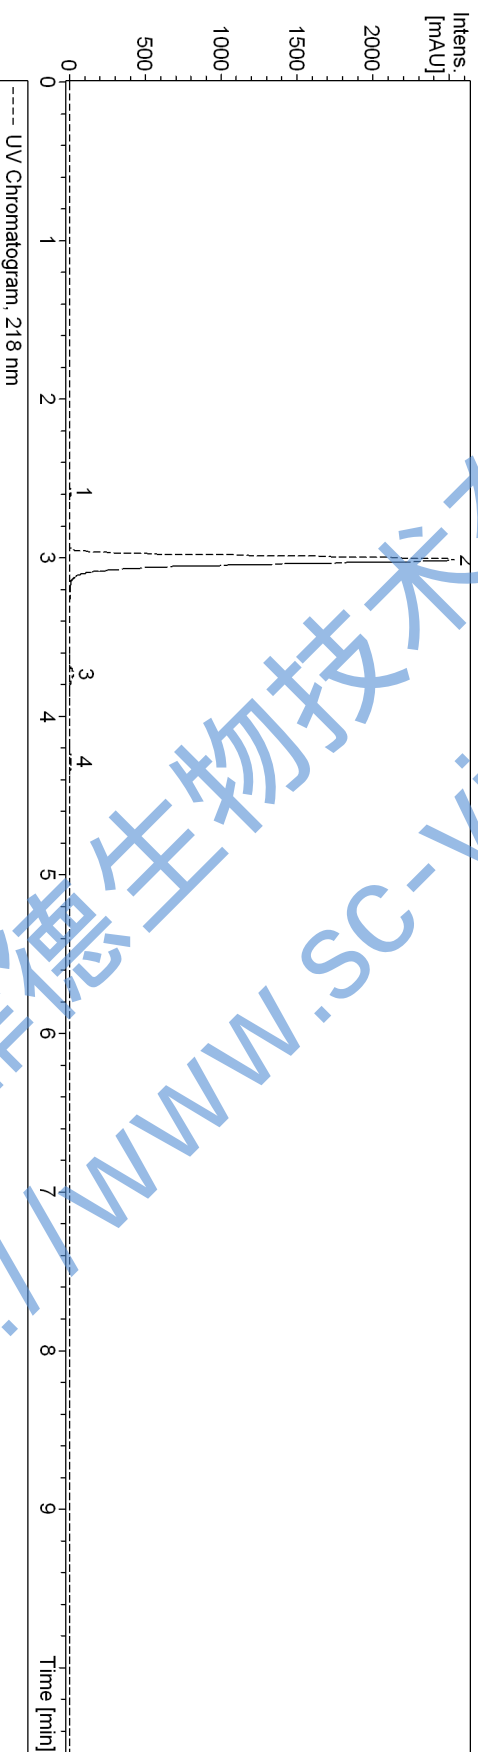

#	RT [min]	Area	Area Frac. %
1	2.6	45.138	0.3
2	3.0	9531.612	98.9
3	3.7	116.110	0.7
4	4.3	71.897	0.1